


## *AD-211 VOC Speciation in Natural Gas, Syngas & Gasification*

### Composition of Natural Gas, Syngas via VOC Speciation

The composition of fuel gas is important in order to determine calorific value and also to detect any unwanted contaminants in the gas. Online analysis is important in order to give real-time and direct action on issues.

#### atmosFIRi Solution

atmosFIRi is a Fourier Transform Infra-Red (FTIR) analyser with a very small volume flow-through cell and a high throughput single pass gas cell. There are no costly gold coated optics with in the gas cell, as long pathlength are not required. The analyser is designed to give quick response to % level concentrations of individual VOCs present within natural gas, biogas and syngas. atmosFIRi is a high resolution measurement, bringing the power of laboratory grade analytics into a robust, stable and easy to maintain process analyser. The high resolution enables complex over-lapping features of multiple VOCs to be detected and quantified.

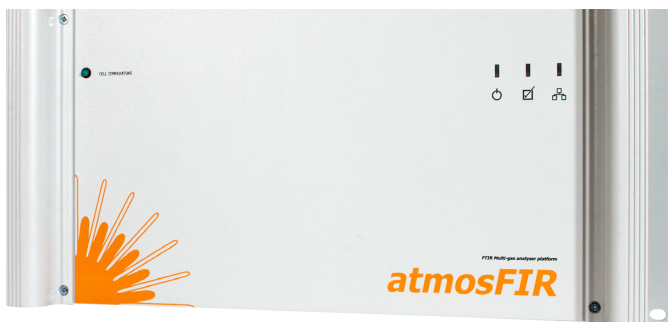

atmosFIRi is supplied with an embedded controller that carries out the complex chemometric analysis of the IR spectra. This is done in real-time and has no limit to the number of gas species that can be identified and quantified.

Measurement results are displayed and trended on-screen and can be reported in ppm or % Vol concentration values. Protea's PAS-Pro software can also be customised to give total summation of individual species. We can also offer in-built calculation to give BTU values. Readings are outputted in real-time via 4-20mA, OPC or Modbus (TCP/IP or serial) connections.

Gas	Lower Detection Limit / Vol%	Minimum Quantifiable Limit in CH4 background / %Vol	Range / %Vol
CH4	0.001	--	0 – 100
CO2	0.1	0.01	0 – 100
CO	0.002	0.01	0 – 100
Ethane	0.002	0.5	0 – 100
Propane	0.002	0.5	0 – 100
Butane	0.002	0.2	0 – 100
Iso-butane	0.002	0.2	0 – 100
Pentane	0.005	0.5	0 – 100
Iso-Pentane	0.005	0.5	0 – 100
Hexane	0.005	0.4	0 – 100
C7+	0.005	0.5	0 – 100
Ethylene	0.005	0.5	0 – 100
Propylene	0.005	0.5	0 – 100
2-Methylpropane	0.005	0.5	0 – 100
2-Methylbutane	0.005	0.5	0 – 100
2,2-Dimethylpropane	0.005	0.5	0 – 100
Cyclohexane	0.005	0.2	0 – 100
Benzene	0.01	0.5	0 - 100

Figure 1 - Detectable Limits in zero gas background and in 100% CH4 background

## Speciation of VOCs

Protea's embedded software is designed to run the latest in chemometric algorithms on the full IR spectra collected by the instrument. These methods are designed to identify and separate overlapping spectral responses for gases of interest.

Our methodology does not use a fixed library and spectra and has no limit to the number of separate gas measurements that can be made. The atmosFIRi platform can measure hundreds of gases simultaneously. Each gas measurement uses its own custom analysis algorithm and so each measurement optimises the calculation for that gas, ensuring linear responses, the reduction of effects from interferences and a better lower detection limit.

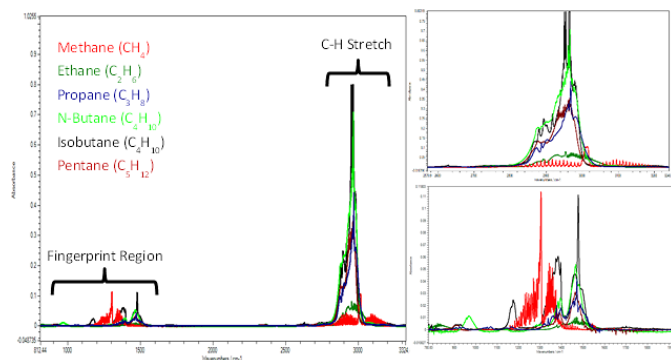


Figure 2 - atmosFIRi spectral responses for VOC across the full infrared spectrum

The benefit of FTIR is that it is a full spectrum analysis technique. This means that we can use both the C-H stretch region (where the C-H stretch bonds common in VOCs are found) and also the fingerprint region, where we can identify unique bonds due to specific functional groups. The full spectrum technique also means that the atmosFIRi analyser can measure CO<sub>2</sub> and CO from ppm to 100% Vol levels, commonly found in syngas.

## Installation and Serviceability

atmosFIRi can be supplied in a 19" rack enclosure, or in a wall-mounted panel configuration. While the basic analyser has to be installed in a non-hazardous area, considerations are made for the sampling of hazardous gas into the equipment as per BS EN 60079-Part 2. Gas flow, containment and dilution principles are all applied to the design.

atmosFIRi contains an easy to remove gas cell assembly. All gas connections are integral to this removable box, so there is no need to make complex plumbed connections inside the unit.

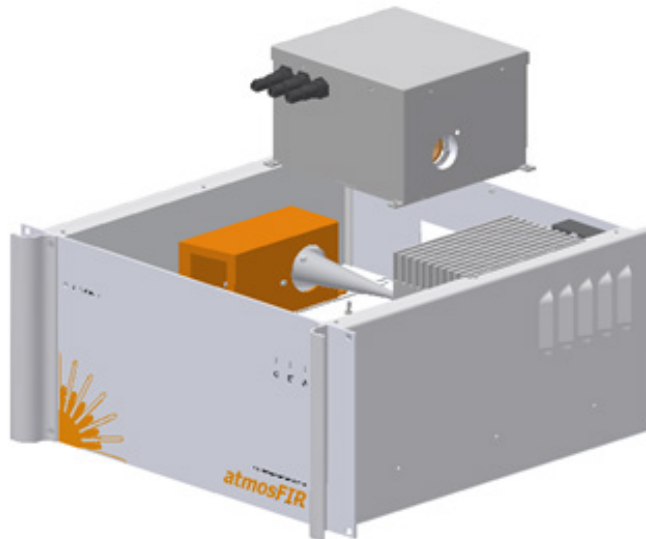


Figure 3 - Removable Gas Cell Box for ease of service

If installation is required in a zoned area, Protea can provide a solution with EX certified enclosure to house the gas analyser.

## Calibration and Repeatability

atmosFIRi does not drift. The IR response is predictable and repeatable. Any variations due to pressure or temperature are measured and controlled within the atmosFIRi electronics. The analyser does not require zero background measurements. Normally these would be achieved with high grade 99.999% Nitrogen, but given the high levels of measurement in gas the zero adjustment can equally be made on air (assuming the VOC content of the zero air is low). atmosFIRi has an in-built solenoid valve for auto-zero.

## Extra Sensing Options

Protea can couple the IR gas composition gas analyser with a number of different sensing options to give total gas measurements. For example, in syngas we can incorporate thermal conductivity sensors for H<sub>2</sub> analysis.

H<sub>2</sub>S is a weak absorber of IR light, and to measure H<sub>2</sub>S we require an additional sensor. This can be achieved with a simple electrochemical sensor, or a high accuracy H<sub>2</sub>S measurement can be determined by parallel measure with our Solus H<sub>2</sub>S TDLAS analyser